





Intended Use

Protects externalized catheters and transmits torque to a swivel for rat infusion or blood sampling. Intended for single use.

Specifications

See <http://www.instechlabs.com/downloads/tethers.pdf>.

Use

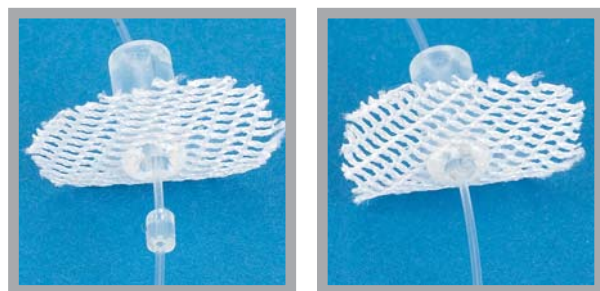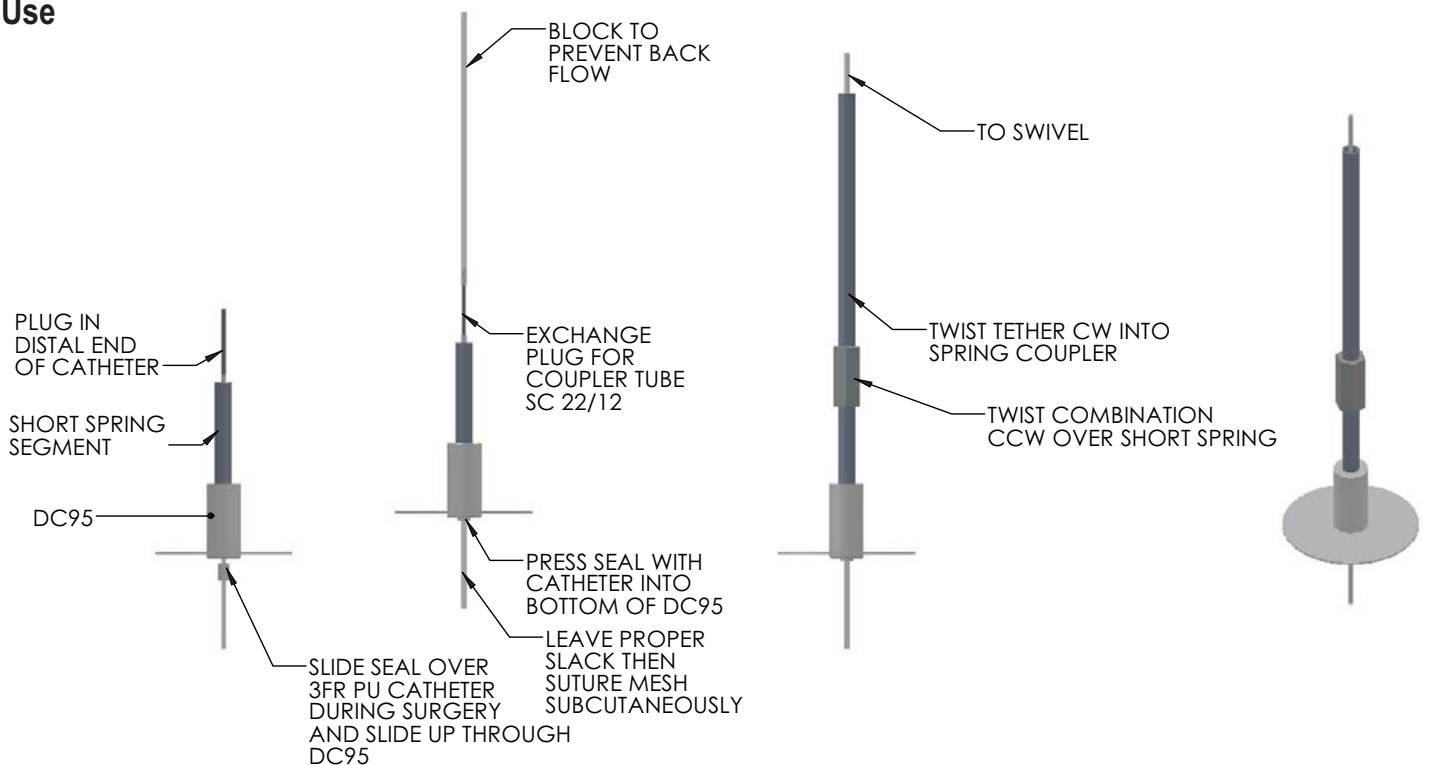

Installation of seal between catheter and button (sized for 3Fr catheters and DC95 buttons only)