



	MODEL NUMBER: PDI-750A/PDI-750XL Individual Power Supply	Document Number: PD196-026R8
	INSTALLATION INSTRUCTIONS	Page 1 of 3

	This symbol indicates that dangerous voltage constituting a risk of electric shock is present within this unit.
	This symbol indicates that there are important operating and maintenance instructions in the literature accompanying this unit.

	CAUTION RISK OF ELECTRIC SHOCK, DO NOT OPEN!	
CAUTION: TO REDUCE THE RISK OF ELECTRIC SHOCK, DO NOT REMOVE COVER. NO USER SERVICEABLE PARTS INSIDE. REFER SERVICING TO QUALIFIED SERVICE PERSONNEL		

THIS INSTALLATION SHOULD BE MADE BY A QUALIFIED SERVICE PERSON AND SHOULD CONFORM TO ALL LOCAL CODES. READ AND FOLLOW THE SAFETY INSTRUCTIONS BEFORE ATTEMPTING THIS INSTALLATION.

	Ce symbole indique qu'une tension dangereuse constituant un risque de choc électrique est présente dans cet appareil.
	Ce symbole indique qu'il existe des instructions d'utilisation et d'entretien importantes dans la documentation accompagnant cet appareil.

	AVERTISSEMENT RESQUE DE CHOC ELECTRIQUE, NE PAS OUVRIR!	
AVERTISSEMENT: AFIN DE REDUIRE LE RISQUE DE CHOC ELECTRIQUE, NE PAS RETIRER LE COUVERCLE, L'APPAREIL NE CONTIENT AUCUN COMPOSNT SUSCEPTIBLE D'ETRE REPAIRE PAR L'UTILISATEUR. CONFIER L'ENTRETIEN A DU PERSONNEL QUALIFIE		

CETTE INSTALLATION DOIT ÊTRE EFFECTUÉE PAR UN TECHNICIEN QUALIFIÉ ET DOIT ÊTRE CONFORME À TOUS LES CODES LOCAUX. LIRE ET SUIVRE LES CONSIGNES DE SÉCURITÉ AVANT DE PROCÉDER À L'INSTALLATION.


Underwriters Laboratories

The power supply models PDI-750A and PDI-750XL are Hospital Grade specialized power supplies and should be installed to National Electrical Code specifications. This device is safety tested and listed by the Underwriters Laboratories as a product suitable for use in health-care facilities in both the United States and Canada.




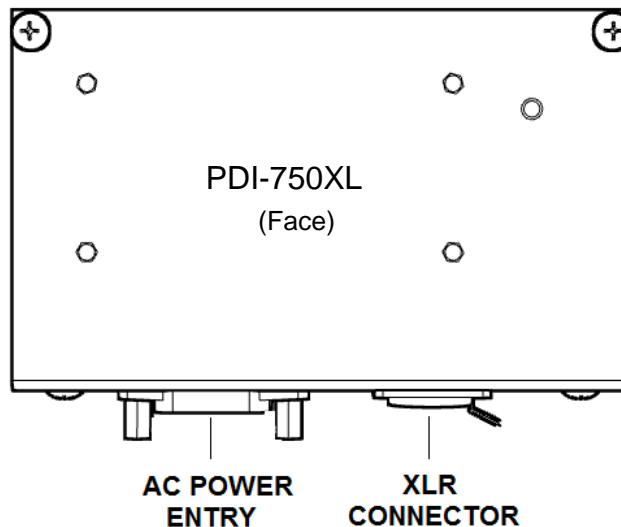
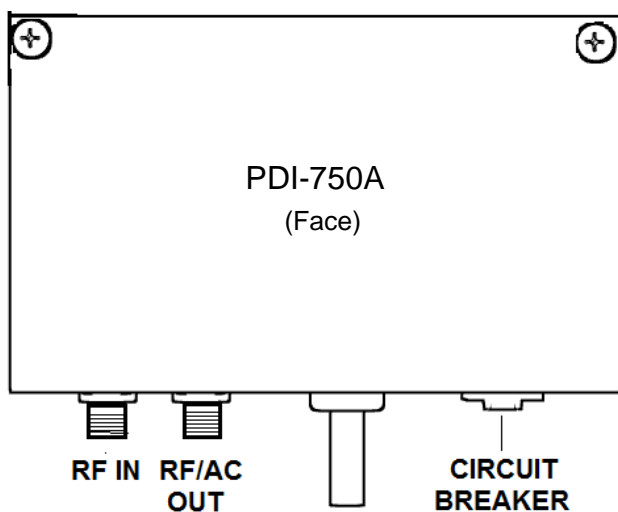
NOTE to CATV system installer:

This reminder is provided to call the CATV system installer's attention to Article 820-40 of the NEC that provides guidelines for proper grounding and, in particular, specifies that the cable ground shall be connected to the grounding system of the building, as close to the point of cable entry as practical.

	MODEL NUMBER: PDI-750A/PDI-750XL Individual Power Supply	Document Number: PD196-026R8
	INSTALLATION INSTRUCTIONS	Page 2 of 3


GUIDELINES

- LOCATION** – Locate a mounting position for the power supply near the suspension arm and an AC wall outlet. Please note that the supply mounts with the AC line cord pointed down.
- MOUNTING TEMPLATE** – Position the mounting template on the desired wall location. Mark the mounting hole locations.
- HARDWARE REQUIREMENTS** – Required hardware for mounting the 750A or 750XL. Hardware is not supplied with the wall bracket.
 DRY WALL – Use two ¼" – 20 toggle bolts.
 MASONRY WALL – Use two ¼" – 20 cement anchors.
 Install the proper wall anchor. Thread both bolts into the wall until approximately ½" of the bolt remains exposed.
- REMOVE COVER** – Remove two screws from the face of the supply at each corner. Save screws. Loosen two screws on the connector area. Lift and separate the cover from the back enclosure. **NOTE:** Use caution, the power supply is mounted to the cover.
- MOUNT ENCLOSURE** – Position exposed bolt heads through the enclosure keyholes.

CERTAIN MODELS WILL HAVE KNOCKOUTS THAT MUST BE REMOVED TO USE THE REAR MOUNTING HOLES IN THE CASTING. REMOVE KNOCKOUTS WITH HAMMER AND PUNCH. POWER SUPPLY MUST BE COMPLETELY DISSASSEMBLED BY REMOVING THE ELECTRONICS SECTION FROM THE CASTING BEFORE INSTALLATION, SEE STEP 4.
 Make certain the enclosure seats properly in each keyhole. It may be necessary to alternately remove the enclosure and tighten or loosen each bolt to bring the enclosure snug against the wall. Tighten both mounting bolts.
- REPLACE COVER** – Reattach the cover to the mounted enclosure making sure the bottom screws seat in the cover with the washers placed between the cover and enclosure. Insert and tighten the two screws located in the face of the supply at the top corners. Tighten the bottom screws.
- CONNECTIONS** – For **PDI-750A**, attach coaxial cable from TV to "F" fitting marked "RF/AC OUT". Attach coaxial cable from Master Antenna TV system to "F" fitting marked "RF IN".
 For **PDI-750XL**, connect XLR from TV. Connect power cable with IEC320-C13 plug which must be purchased separately.
- POWER** – For **PDI-750A**, plug AC line cord into 120 VAC outlet. For **PDI-750XL**, plug AC line cord into 120/240 VAC outlet.



PDi <small>Communication Systems, Inc.</small> <i>Better Solutions Are Within Reach®</i>	MODEL NUMBER: PDI-750A/PDI-750XL Individual Power Supply	Document Number: PD196-026R8
	INSTALLATION INSTRUCTIONS	Page 3 of 3

TOP



POWER SUPPLY MOUNTING TEMPLATE

PDI-750A – SPECIFICATIONS

Input	120VAC, 60HZ, 1A
Output	28VAC, 3.5A
Insertion Loss (50MHz – 850MHz)	<2dB
Return Loss (50MHz – 850MHz)	>6dB

PDI-750XL – SPECIFICATIONS

Input	100-240VAC, 50/60HZ, 2A
Output	12VDC, 5A